



ichroma™ Cortisol

INTENDED USE

ichroma™ Cortisol is a fluorescence Immunoassay (FIA) for the quantitative determination of Cortisol in human whole blood/serum/plasma. It is useful as an aid in management and monitoring of concentration of cortisol.

For *in vitro* diagnostic use only.

INTRODUCTION

Cortisol is a potent hormone known as a glucocorticoid that affects the metabolism of carbohydrates, proteins, and fats, but especially glucose. Cortisol test is performed on patients who may have malfunctioning adrenal glands. Cortisol level normally rises and falls during the day. It peaks its highest level between 6 and 8 AM and gradually falls, reaching its lowest point around midnight. When cortisol level is measured, blood specimen is usually collected at 8 AM and again at 4 PM. It should be noted that normal values may be adjusted in individuals who have worked during the night and slept during the day for long periods of time. **ichroma™ Cortisol** quantitatively measures the cortisol concentration of whole blood, serum and plasma.

PRINCIPLE

The test uses a competitive immunodetection method.

In this method, the target material in the sample binds to the fluorescence (FL)-labeled detection antibody in detection buffer, to form the complex as sample mixture. This complex is loaded to migrate onto the nitrocellulose matrix, where the covalent couple of cortisol and bovine serum albumin (BSA) is immobilized on a test strip, and interferes with the binding of target material and FL-labeled antibody. If the more target material exists in blood, the less detection antibody is accumulated, resulting in the less fluorescence signal.

COMPONENTS

ichroma™ Cortisol consists of 'Cartridges', 'Detection Buffer Tubes' and an 'ID chip'.

- The cartridge contains a test strip, the membrane which has BSA-human cortisol at the test line, while streptavidin at the control line.
- Each cartridge is individually sealed in an aluminum foil pouch containing a desiccant. 25 sealed cartridges are packed in a box which also contains an ID chip.
- The detection buffer contains anti human cortisol-fluorescence conjugate, biotin-BSA-fluorescence conjugate, bovine serum albumin (BSA) as a stabilizer and sodium azide in phosphate buffered saline (PBS) as a preservative.
- The detection buffer is dispensed in a tube. 25 detection buffer tubes are packaged in a box and further packed in a Styrofoam box with ice-pack for the shipment.

WARNINGS AND PRECAUTIONS

- For *in vitro* diagnostic use only.
- Carefully follow the instructions and procedures described in this 'Instructions for use'.
- Use only fresh samples and avoid direct sunlight.
- Lot numbers of all the test components (cartridge, ID chip and detection buffer) must match each other.
- Do not interchange the test components between different lots

or use the test components after the expiration date, either of which might yield misleading of test result(s).

- Do not reuse. A detection buffer tube should be used for processing one sample only. So should a cartridge.
- The cartridge should remain sealed in its original pouch before use. Do not use the cartridge, if it is damaged or already opened.
- Frozen sample should be thawed only once. For shipping, samples must be packed in accordance with the regulations. Sample with severe hemolytic and hyperlipidemia cannot be used and should be recollected.
- Just before use, allow the cartridge, detection buffer and sample to be at room temperature for approximately 30 minutes.
- **ichroma™ Cortisol** as well as the instrument for **ichroma™** tests should be used away from vibration and/or magnetic field. During normal usage, it can be noted that instrument for **ichroma™** tests may produce minor vibration.
- Used detection buffer tubes, pipette tips and cartridges should be handled carefully and discarded by an appropriate method in accordance with relevant local regulations.
- An exposure to larger quantities of sodium azide may cause certain health issues like convulsions, low blood pressure and heart rate, loss of consciousness, lung injury and respiratory failure.
- **ichroma™ Cortisol** will provide accurate and reliable results subject to the following conditions.
 - Use **ichroma™ Cortisol** should be used only in conjunction with instrument for **ichroma™** tests.
 - Any anticoagulants other than EDTA should be avoided.

STORAGE AND STABILITY

- The cartridge is stable for 20 months (while sealed in an aluminum foil pouch) if stored at 4-30 °C.
- The detection buffer dispensed in a tube is stable for 20 months if stored at 2-8 °C.
- After the cartridge pouch is opened, the test should be performed immediately.

LIMITATION OF THE TEST SYSTEM

- The test may yield false positive result(s) due to the cross-reactions and/or non-specific adhesion of certain sample components to the capture/detector antibodies.
- The test may yield false negative result. The non-responsiveness of the antigen to the antibodies is most common where the epitope is masked by some unknown components, so as not to be detected or captured by the antibodies. The instability or degradation of the antigen with time and/or temperature may cause the false negative as it makes antigen unrecognizable by the antibodies.
- Other factors may interfere with the test and cause erroneous results, such as technical/procedural errors, degradation of the test components/reagents or presence of interfering substances in the test samples.
- Any clinical diagnosis based on the test result must be supported by a comprehensive judgment of the concerned physician including clinical symptoms and other relevant test results.

MATERIALS SUPPLIED

REF CFPC-24

Components of **ichroma™ Cortisol**

- Cartridge Box:
 - Cartridges 25
 - ID Chip 1
 - Instruction For Use 1
- Box containing Detection Buffer tubes
 - Detection Buffer Tubes 25

MATERIALS REQUIRED BUT SUPPLIED ON DEMAND

Following items can be purchased separately from **ichroma™ Cortisol**. Please contact our sales division for more information.

- Instrument for ichroma™ tests
 - **ichroma™ Reader** [REF] FR203
 - **ichroma™ II** [REF] FPRR021
 - **ichroma™ D** [REF] 13303
- **ichroma™ Printer** [REF] FPRR007
- **Boditech Hormone Control** [REF] CFPO-95

SAMPLE COLLECTION AND PROCESSING

The sample type for **ichroma™ Cortisol** is human whole blood/serum/plasma.

- It is recommended to test the sample within 24 hours after collection.
- The serum or plasma should be separated from the clot by centrifugation within 3 hours after the collection of whole blood. If longer storage is required, e.g. if the test could not be performed within 24 hours, serum or plasma should be immediately frozen below -20 °C. The freezing storage of sample up to 3 months does not affect the quality of results
- However, the whole blood sample should not be kept in a freezer in any case.
- Once the sample was frozen, it should be used one time only for test, because repeated freezing and thawing can result in the change of test values.

TEST SETUP

- Check the contents of **ichroma™ Cortisol**: Sealed Cartridge, Detection Buffer Tubes and ID Chip.
- Ensure that the lot number of the cartridge matches that of the ID chip as well as the detection buffer.
- Keep the sealed cartridge (if stored in refrigerator) and the detection buffer tube at room temperature for at least 30 minutes just prior to the test. Place the cartridge on a clean, dust-free and flat surface.
- Turn on the instrument for ichroma™ tests.
- Insert the ID Chip into the ID chip port of the instrument for ichroma™ tests.
- Press the 'Select' button on the instrument for ichroma™ tests. (Please refer to the 'Instrument for ichroma™ tests Operation Manual' for complete information and operating instructions.)

CAUTION

- To minimize erroneous test results, we suggest that the ambient temperature of the cartridge should be 25 °C during the reaction time after loading sample mixture to the cartridge.
- To maintain the ambient temperature to 25 °C, you can use various devices such as an i-Chamber or an incubator and so on.

TEST PROCEDURE

- 1) Transfer 30 µL (Human serum/plasma/control) or 50 µL (Human whole blood) of sample using a transfer pipette to a tube containing the detection buffer.
- 2) Close the lid of the detection buffer tube and mix the sample thoroughly by shaking it about 10 times. (The sample mixture must be used immediately.)
- 3) Pipette out 75 µL of a sample mixture and load it into the sample well on the cartridge.
- 4) Insert the sample-loaded cartridge into the slot of the i-Chamber or an incubator (25 °C).
- 5) Leave the sample-loaded cartridge in the i-Chamber or an incubator for 10 minutes.
 ▲ Scan the sample-loaded cartridge immediately when the incubation time is over. If not, it will cause inexact test result.
- 6) To scan the sample-loaded cartridge, insert it into the cartridge

holder of the instrument for ichroma™ tests. Ensure proper orientation of the cartridge before pushing it all the way inside the cartridge holder. An arrow has been marked on the cartridge especially for this purpose.

- 7) Press 'Select' button on the instrument for ichroma™ tests to start the scanning process.
- 8) Instrument for ichroma™ tests will start scanning the sample-loaded cartridge immediately.
- 9) Read the test result on the display screen of the instrument for ichroma™ tests.

INTERPRETATION OF TEST RESULT

- Instrument for ichroma™ tests calculates the test result automatically and displays cortisol concentration of the test sample in terms of nmol/L.
- Reference range
 - Morning: 140-700 nmol/L
 - Midnight: 80-350 nmol/L
- Working range: 80-800 nmol/L

QUALITY CONTROL


- Quality control tests are a part of the good testing practice to confirm the expected results and validity of the assay and should be performed at regular intervals.
- The control tests should be performed immediately after opening a new test lot to ensure the test performance is not altered.
- Quality control tests should also be performed whenever there is any question concerning the validity of the test results.
- Control materials are not provided with **ichroma™ Cortisol**. For more information regarding obtaining the control materials, contact **Boditech Med Inc.'s Sales Division for assistance**. (Please refer to the instruction for use of control material.)

PERFORMANCE CHARACTERISTICS

- **Specificity:** There, in test samples, are biomolecules such as cortisone, corticosterone, prednisolone, progesterone, prednisone, deoxycortisol, testosterone, dHEA, and dexamethasone in higher concentration than their normal physiological levels. But this doesn't interfere with the **ichroma™ Cortisol** test measurements, nor occurs any significant cross-reactivity.
- **Precision:** The intra-assay precision was calculated by one evaluator, who tested different concentration of control standard 20 times each with three different lots of **ichroma™ Cortisol**. The inter-assay precision was confirmed by 3 different evaluators with 3 different lots, testing 3 times each different concentration.

Cortisol [nmol/L]	Intra-assay		Inter-assay	
	Mean	CV (%)	Mean	CV (%)
95.2	96.6	5.4	96.2	5.6
205.1	201.7	4.11	204.6	5.4
346.0	352.0	5.21	348.4	5.7
573.6	575.51	4.27	576.4	5.5

- **Comparability:** Cortisol concentrations of 60 clinical samples were quantified independently with **ichroma™ Cortisol** and BioMerieux mini VIDAS as per prescribed test procedures. Test results were compared and their comparability was investigated with linear regression and coefficient of correlation (R). Linear regression and coefficient of correlation between the two tests were $Y=0.988X - 18.608$ and $R = 0.923$ respectively.

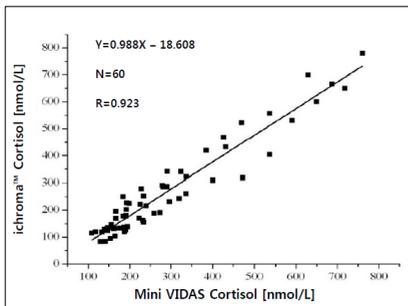

REFERENCES

1. Gustavo, E.T. Correlation between cortisol level and serotonin uptake in patients with chronic stress and depression. *Cognitive, Affective, & Behavioral Neuroscience* 2001, 1(4): 388-393.
2. Sonia, J.L., Mony, L., Susan, S., Antonio, A., Chaim, T., Mira, T., Bruce, S., M., Richard, L.H., and Michael, J.M. Cortisol levels during human aging predict hippocampal atrophy and memory deficits. *Nature* 1998, 1:69-73.
3. Bartels, M., Van den Berg, M., Sluyter, F., Boomsma, D.I., de Geus, E.J.C. Heritability of cortisol levels: review and simultaneous analysis of twin studies. *Psychoneuroendocrinology* 2003, 28:121-137.

Note: Please refer to the table below to identify various symbols

	Sufficient for <n> tests
	Read instruction for use
	Use by Date
	Batch code
	Catalog number
	Caution
	Manufacturer
	Authorized representative of the European Community
	In vitro diagnostic medical device
	Temperature limit
	Do not reuse
	This product fulfills the requirements of the Directive 98/79/EC on in vitro diagnostic medical devices

For technical assistance; please contact:

Boditech Med Inc.'s Technical Services

Tel: +82 33 243-1400

E-mail: sales@boditech.co.kr



Boditech Med Incorporated

43, Geodudanji 1-gil, Dongnae-myeon,
 Chuncheon-si, Gang-won-do, 24398
 Republic of Korea

Tel: +(82) -33-243-1400

Fax: +(82) -33-243-9373

www.boditech.co.kr



Obelis s.a

Bd. Général Wahis 53,
 1030 Brussels, BELGIUM

Tel: +(32) -2-732-59-54

Fax: +(32) -2-732-60-03

E-Mail: mail@obelis.net

